

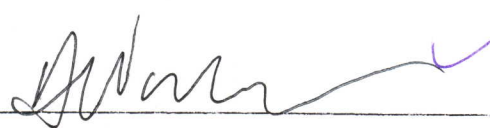
# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

MAR 20 2010

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130305 ✓
Name		Anthony Wallace	ID# 6555 Date 3/22/10 ✓
A	Agency	Hoonah Police Department	Phone # 945-3655
Instrument Location		Hoonah Police Department ✓	
Alco S/N		X 301532 ✓	Target Value .082 ✓ High Pressure
B	Alco Test Value Average	.088 ✓	.089 ✓
		1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco
Signature			
(OVER)			

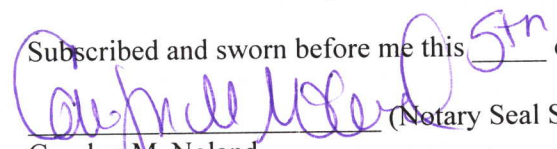
BMB  
4/1/10

I, Nita J. Bolz, after being first duly sworn, depose and state as follows: (Do Not write in the area below)

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 5<sup>th</sup> day of April, 2010.

  
(Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130305

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130305

MARCH 22, 2010

OPERATOR'S NAME:  
WALLACE ANTHONY  
OPERATOR'S NUMBER: 6555  
SUBJECT'S LAST NAME:  
VOC

SUBJECT'S FIRST NAME/MI :  
VOC

O.L. #: VOC  
DEPT/AGENCY: HNH1  
CASE/REPORT: VOC  
TEST TYPE: U

ALCO TARGET VALUE: .082  
ALCO S/N: K301532

### --- BREATH ANALYSIS ---

.082 ADJUSTED FOR 30.06 in  
ALCO TARGET .082 03:00  
BLANK TEST .000 03:01  
INTERNAL STANDARD VERIFIED 03:01  
ALCO TV 30.06 in .088 03:01  
BLANK TEST .000 03:02  
SUBJECT SAMPLE .000 03:03  
BLANK TEST .000 03:03  
ALCO TV 30.06 in .088 03:04  
BLANK TEST .000 03:04

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130305

MARCH 22, 2010  
TIME 02:55

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 01/08/09  
HEATERS  
SAMPLE CHAMBER: 48c  
BREATH TUBE: 42c  
BAROMETER: 30.06 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEF6  
HIJKLHNOPIQRSTUUVWXYZ[\]^\_`abcdefghijklmnopqrstuvwxyz{|}~